

10019743.102501



## Implantable Cardiac Therapy Device with Dual Chamber Can to Isolate High-Frequency Circuitry



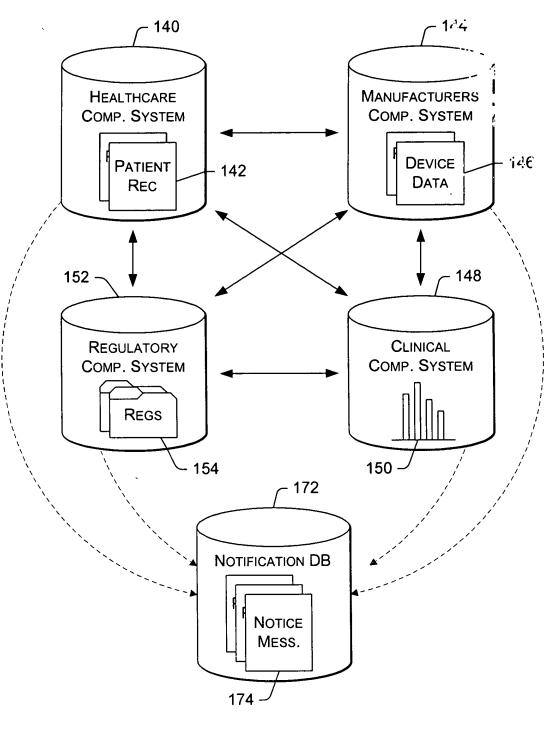


Fig.3



HOOMS/AN HORSCH

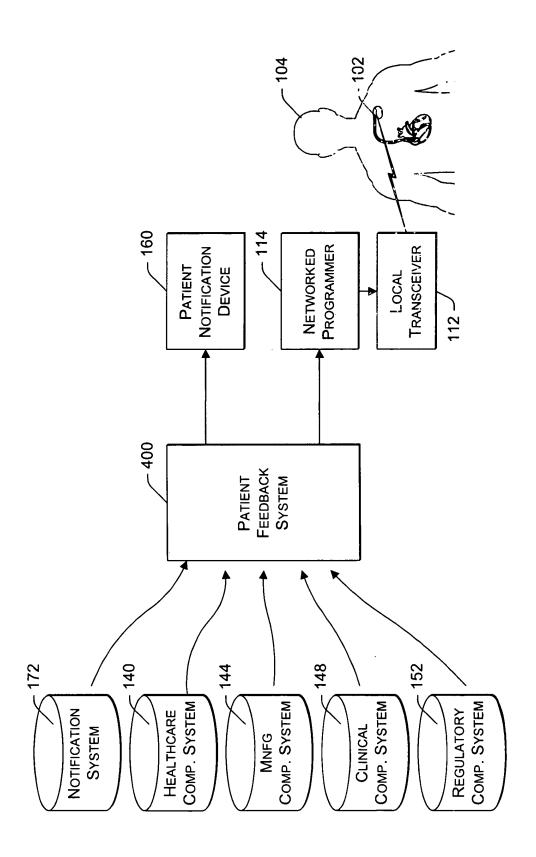



Implantable Cardiac Therapy Device with Dual Chamber Can to Isolate High-Frequency Circuitry

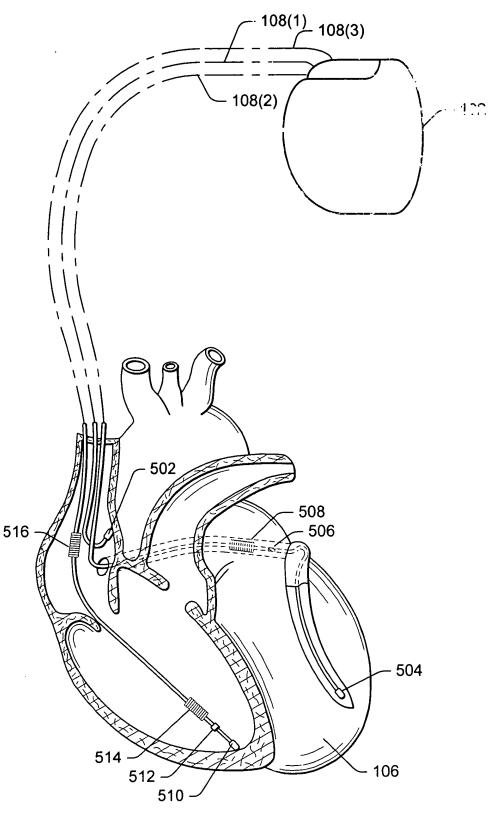
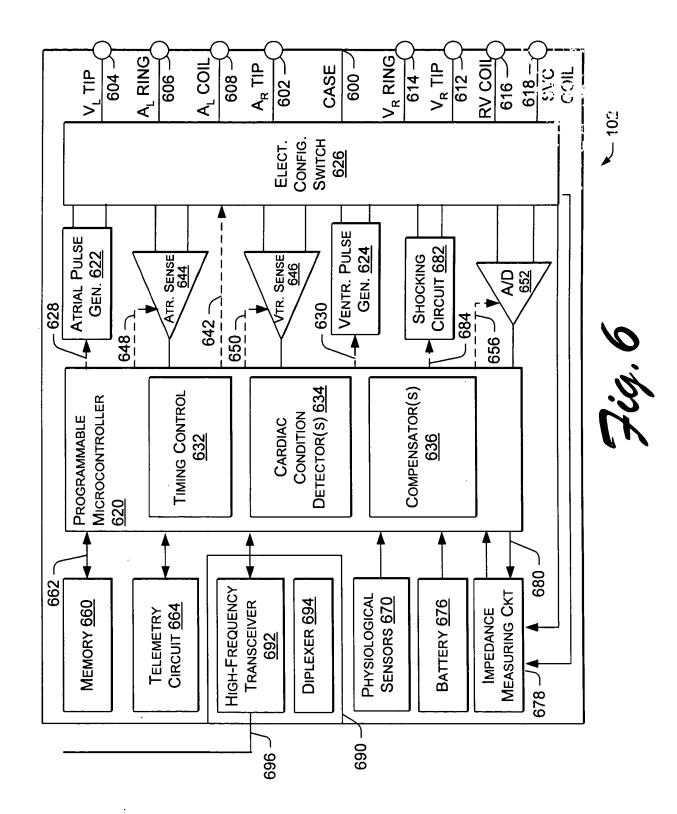


Fig.5

SJ1-026US / A00E1220
Shankar et al.
Implantable Cardiac Therapy Device with Dual Chamber Can to Isolate High-Frequency Circuitry



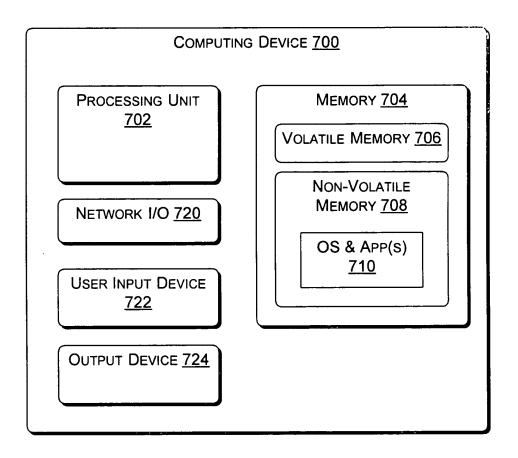


Fig. 7

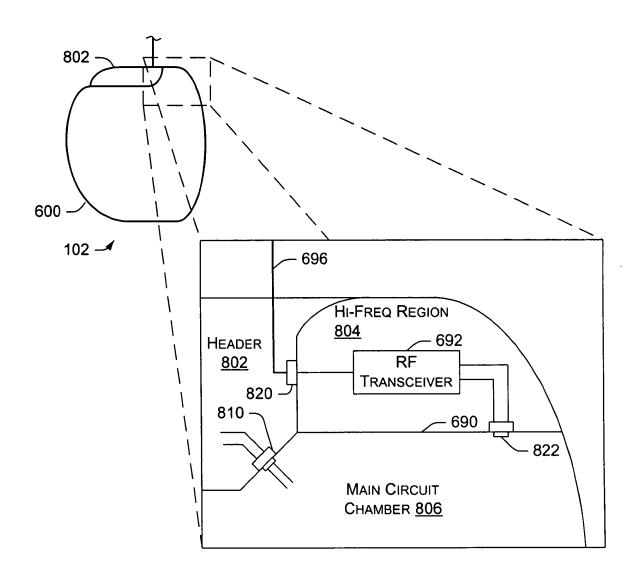


Fig. 8

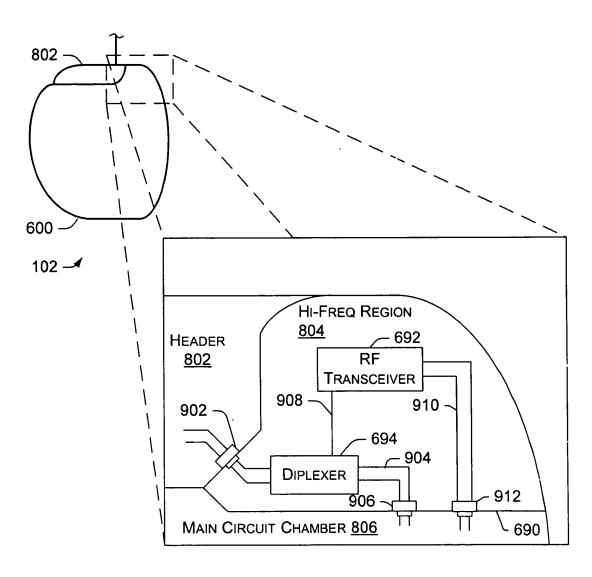
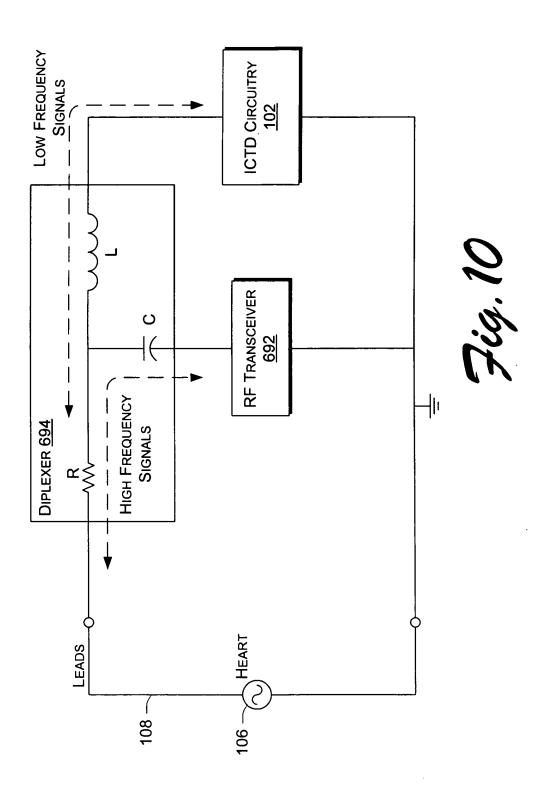
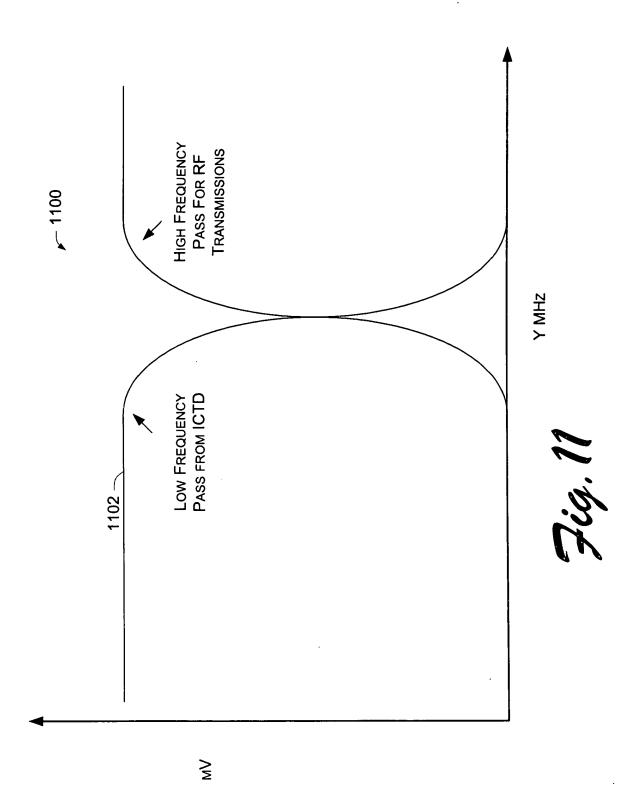


Fig. 9





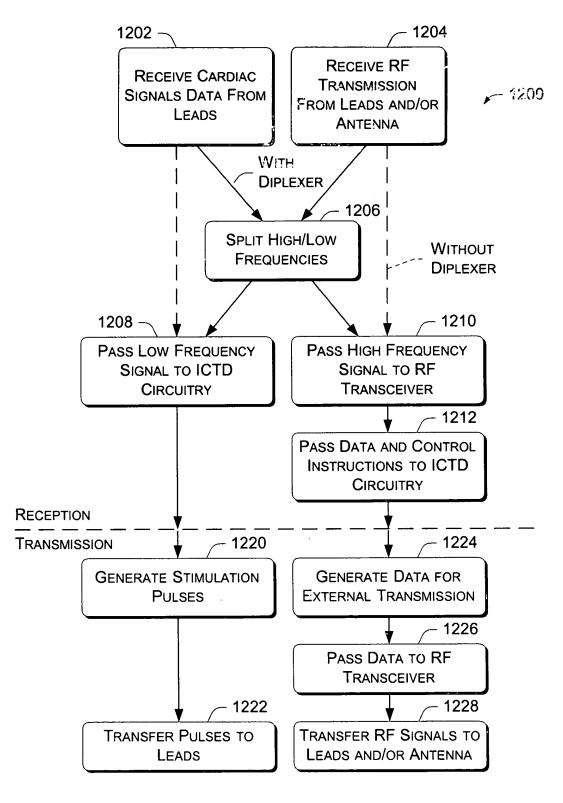


Fig. 12